

Original Research

# An Airborne Fungal Spore Mass Measurement System Based on Graphene Oxide Coated QCM

Arif Budianto<sup>1,2</sup>, Arinto Yudi Ponco Wardoyo<sup>1</sup>, Masruroh<sup>1</sup>,  
Hari Arief Dharmawan<sup>1</sup>

<sup>1</sup>Physics Department, Brawijaya University, Jl. Veteran 65145 Malang, East Java, Indonesia

<sup>2</sup>Physics Study Program, Mataram University, Jl. Majapahit 62 Mataram, West Nusa Tenggara, Indonesia

Received: 8 November 2021

Accepted: 3 March 2022

## Abstract

This study aims to develop a real-time QCM (quartz crystal microbalance)-based method for a fungal spore mass measurement system as the indoor air pollutants. *Penicillium camemberti* (B2), *Penicillium caseifulvum* (B3), and a mixture of both *P. camemberti* and *P. caseifulvum* (B4) were used as the bioaerosol samples in the form of fungal spores. These samples were collected and cultured inside an isolated chamber and mixed with fresh air (filtered by a filter paper) to generate bioaerosol with a diameter of less than 1  $\mu\text{m}$  (fine particles). These bioaerosols were filtered to produce different particle diameters using a particulate cyclone (a filter paper and a suction pump). The developed system consisted of a GO (graphene oxide, a graphene derivative)-coated QCM (Q1), a bare QCM (Q2), a crystal oscillator, and a frequency counter to process the output signal, QCM's frequency, and bioaerosol mass. The system shows a good performance with the sensitivity of  $27 \times 10^{-2}$  to  $29 \times 10^{-2}$  Hz/ng and  $23 \times 10^{-2}$  to  $29 \times 10^{-2}$  Hz/ng for coated and uncoated sensors, respectively. The best performance is obtained from the coated QCM sensor Q1. The system works well in measuring bioaerosol concentrations with an accuracy of 82% for the coated QCM and 66% for the uncoated QCM. The coated QCM has the potentials of being developed as a fungal spore sensor.

**Keywords:** fungal spores, graphene oxide, indoor air pollutant, measurement system, quartz crystal microbalance

## Introduction

Bioaerosols are the biological constituent of PM (particulate matter). Bioaerosols are produced during many activities in landfills, agricultural sectors, food preservation, and many others in daily life [1, 2]. Bioaerosols can be generated from biomass burning

activity, resulting in bioaerosols with a diameter  $< 2.5 \mu\text{m}$  (fine bioaerosols) [2]. Bioaerosols commonly have many forms like fungal spores, pollen, bacteria, and even viruses. As confirmed before, bioaerosols consist of *Aspergillus*, *Alternaria*, and *Cladosporium* species [4, 5]. Another previous study investigated bioaerosols from bacteria species in landfill areas, such as *Staphylococcus aureus*, *Staphylococcus gordonii*, *Alloicoccus otitis*, *Kocuria rosea*, *Pediococcus pentosaceus*, and many others [1].

\*e-mail: a.wardoyo@ub.ac.id

Fungal spores are one common kind of bioaerosol that may adversely affect human health and the environment. Some fungal spores can cause allergic asthma [6, 7]. Another study shows the individual effects of the daily exposure to *Alternaria* and *Cladosporium* species as the biological constituents of PMs to the lung function in schoolchildren [7]. Especially for *Penicillium sp.*, this bioaerosol can be found indoors as mold, with different species such as *Penicillium crustosum*, *Penicillium chrysogenum*, and *Penicillium brevicompactum* [8].

Fungal spores concentration can be measured using many techniques. They can be measured using an indirect measurement, such as a real-time polymerase chain reaction [9]. Particle number concentrations of bioaerosols can also be measured using a scanning mobility particle sizer (SMPS) or an optical particle sizer (OPS) [10]. Another study used UV-APS (ultraviolet aerodynamic particle sizer) to measure bacterial aerosols, such as *Staphylococcus epidermis* and *Escherichia coli* [11]. These measurement systems are not portable, are high cost, generally use indirect measurement, and need extra maintenances or specialized training.

A quartz crystal microbalance (QCM) sensor can measure a nanogram-scale change in mass among various measurement methods by recording its frequency shift. This sensor has been widely used due to its real-time performance, high sensitivity, ease of installation, and low cost [12, 13]. Thus far, this sensor has a resonator surface that can be modified as a sensitive layer related to its function. For sensitivity purposes, a QCM sensor needs specific coating material on the surface of its electrode. For example, a previous study fabricated QCM sensors using polystyrene particles coated with transferrin to predict nanoparticle in vivo behavior [14].

Recently, graphene has been studied as a coating material due to its superior electronic conductivity and high thermal stability [15]. The graphene oxide (GO) nanosheet (thin film for coating material) has good hydrophilicity, specific surface areas, and dispersion stability, as GO is the graphene derivatives [12]. GO inherently represents a good mechanical modulus which may cause a small probability of the swelling effect (false crystal frequency response due to over mass) that influences the QCM response [16]. GO has been used as a specific coating material in QCM and utilized for many sensors. GO-coated QCM has a good response in sensing formaldehyde concentration [17]. As a composite, GO/ polydopamine has been developed as a good humidity sensing device due to its ultra-sensitive behavior in water contents [12]. As a gas sensor, GO/TiO<sub>2</sub> composites can be deposited on the QCM's surface [15]. Bioaerosol hazard measurement research is still at an early stage. Since fungal and other bioaerosols have mycotoxins, accurate and sensitive analytical methods are urgently required. These kinds of particulate matter are also easily spread and suspended

in ambient air, making them easier to breathe and may increase respiratory health problems. Our study aims to develop a bioaerosol measurement system based on a QCM sensor and to identify the performance of a graphene oxide-coated QCM for a fungal spore sensor.

## Materials and Methods

### Measurement System

This study used a microcontroller (Atmega 328), self-developed crystal oscillators (maximum crystal input = 16 MHz of frequency  $f$ ), QCM sensors (uncoated and GO-coated AT-cut QCMs, fundamental frequency = 5.0 MHz), and suction pumps (1.0 m/s of the flowrate) as the main parts of the developed system. According to the preliminary study, the best suction pump flow rate was lower than 2.0 m/s [18]. These parts were integrated inside a polycarbonate prototype box (15 cm (length) x 15 cm (width) x 8 cm (height)). Both QCMs were placed inside a sensor box and connected to the oscillators to drive the signal. The signals from the output pins were connected to the microcontroller to process the output signals (Fig. 1). The microcontroller worked as the frequency counter that counted the given frequency and changed them into bioaerosol mass. The input and output suction pumps were controlled to suck the bioaerosol sample into the sensor box.

### Bioaerosol Concentrations

This study used filtered fresh air (B1) and three fungal spores as bioaerosol samples. They were *Penicillium camemberti* (B2), *Penicillium caseifulvum* (B3), and a mixture of both *P. camemberti* and *P. caseifulvum* (B4), which were purchased from a local distributor. The fungal samples were cultivated inside a chamber (20 cm (width) x 30 cm (length) x 20 cm (height)) and cultured on potato dextrose agar (PDA, Merck, 1.10130.0500) using glass Petri dishes (dimension: 9 cm x 1.5 cm) for a week at room temperature. *Penicillium sp.* were chosen for safety purposes, with low mycotoxin productions and the cheese strain, and their existence as indoor air pollution substances [19, 20]. After incubation, the fungal spores were injected into an exposure chamber and mixed with fresh air (filtered air using a HEPA filter, 2.1 m/s of the air flowrate using a suction pump) for 60 seconds to identify the sensing capability of the developed system [21].

### Sensor Preparation

This study used GO-coated (Q1) and uncoated QCM (Q2) sensors (fundamental frequency  $f_0 = 5$  MHz, AT-cut, purchased from PT. Great Microtama Electronics Indonesia). These sensors had a diameter of

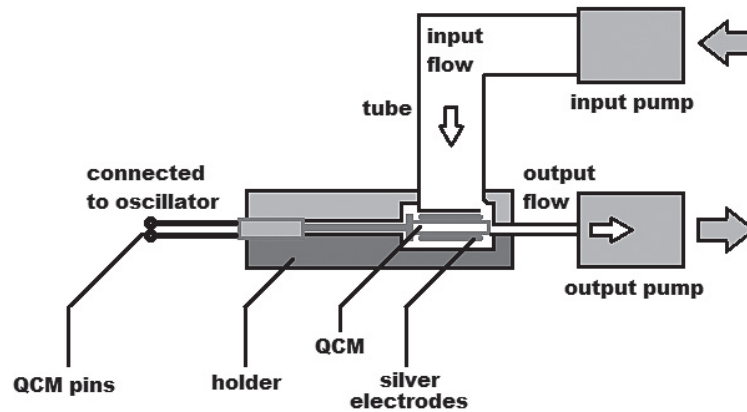


Fig. 1. Schematic diagram of the measurement system.

8.7 mm (silver electrode). All QCM samples were tested before being used and placed in a dust-free box. Each QCM was mounted on a holder made with polylactide and polycarbonate and then connected to a self-made oscillator module [18]. The output signal was then connected to the frequency counter circuit and laptop. The QCM's mountings or holders were also made for the input and output flows and connected to suction pumps (Fig. 1) (modified from Kleo et al. [22]).

#### Measurement Set-Up

All measurements and treatments were conducted inside an experimental chamber. The fungal spores were introduced to the chamber using a suction pump for 60 seconds (modified from Wardoyo et al. [23]) with a flow rate of 2.0 m/s. A filter paper (Whatman™ filter paper Grade 5) was installed on the pump's outlet to allow bioaerosol diameter  $\leq 1.0 \mu\text{m}$  to pass through the filter. In line with this, each bioaerosol sample, including B1, was exposed to the chamber. The bioaerosol concentrations were measured by evaluating the developed system's frequency shift ( $\Delta f$ ) until the value of  $\Delta f$  was stagnant [18]. The bioaerosol concentrations were also measured using a Kanomax Digital Dust Monitor Model 3443.

#### System Performances

Sensitivity ( $S$ ) was evaluated by measuring the frequency shift and varying the bioaerosol samples from B2 to B4 [24]. Since low concentration was not easy to evaluate, the injection time was determined as 110 seconds for a minimum bioaerosol concentration. These tests were conducted at a fixed room temperature at  $\pm 25\text{-}26^\circ\text{C}$ . The following equation was used to calculate  $S$ :

$$S = \Delta f / m \quad (1)$$

System accuracy was investigated by comparing the results with the Digital Dust Monitor.

#### Statistical Analysis

The collected data were presented as the mean value and standard error of the means (SEM). Differences between groups were evaluated using the Analysis of Variance (ANOVA) test. All tests were conducted at  $p < 0.05$  [25].

#### Results

##### Bioaerosol Mass Measurement

Fig. 2 shows the bioaerosol concentration measurement results from Q1 as the coated QCM (Fig. 2a) and Q2 (Fig. 2b), the uncoated QCM. According to the results of the Q1 group, B1, B2, and B3 have bioaerosol concentrations of  $221 \pm 17$ ,  $248 \pm 15 \mu\text{g}/\text{m}^3$ , and  $257 \pm 30 \mu\text{g}/\text{m}^3$ , respectively. Meanwhile, no significantly different results can be seen in B4 with the concentration of  $266 \pm 9 \mu\text{g}/\text{m}^3$ . In Q2, the measurement results show similar concentrations for B1, B2, B3, and B4, resulting in  $229 \pm 16$ ,  $252 \pm 16$ ,  $257 \pm 25$ , and  $263 \pm 5 \mu\text{g}/\text{m}^3$ , respectively. Fig. 2 shows that the filtered air has the lowest concentration. These results are obtained consistently for all repetitions.

The bioaerosol masses ( $m$ , Table 1) were calculated (Eq. (2)) by multiplying the total flow rate ( $\Sigma Q$ ), sampling duration time  $t$ , and total concentration per bioaerosol sample ( $\Sigma C_i$ ). According to the experiment results, the measurement of the particulate concentrations needed 110 seconds of the total sampling time  $t$  to reach the ambient concentration  $C_0$ . Besides, the total flow rate is obtained from the measurement device and the suction pump flow rates ( $44.93 \text{ cm}^3/\text{second}$ ). As expected, the most exposed bioaerosol mass is referred to as B2-B4. The results show no significant difference between Q1 and Q2 sensor groups for all samples ( $p = 0.36$ ). These values are then used to compare the calibrated measurement device and the developed system to get the accuracy level.

$$m = \Sigma Q \cdot \Sigma C_i \cdot t \quad (2)$$

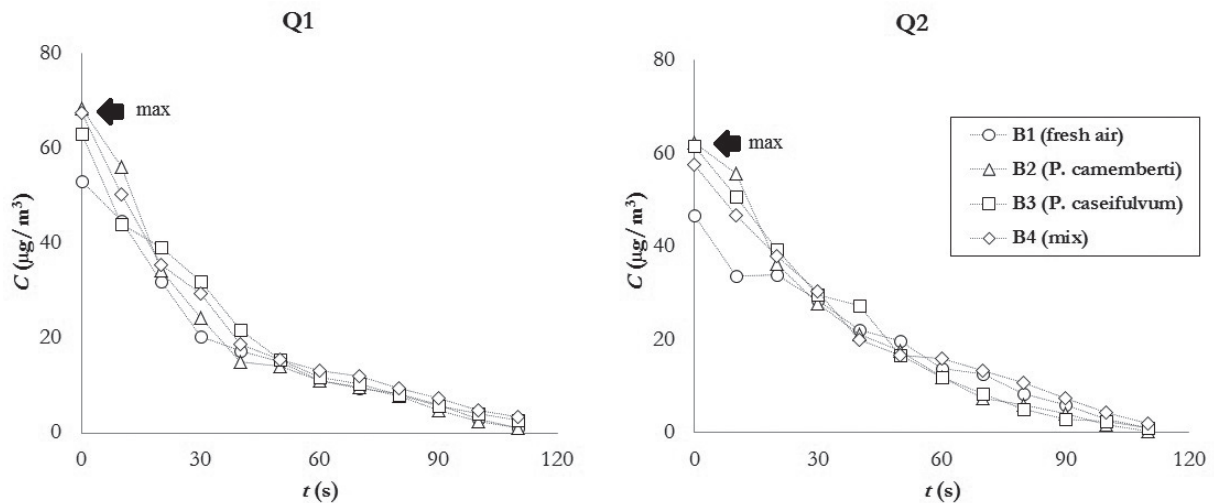


Fig. 2. Measurement results of bioaerosol concentrations ( $C$ ) of all samples (B1-B4) with a diameter  $\leq 1 \mu\text{m}$  (mean): Q1 (GO-coated QCM) and Q2 (uncoated QCM).

Table 1. Exposed sample masses were obtained from Q1 (GO-coated QCM) and Q2 (uncoated QCM).

QCMs	Mass ( $\times 10^{-4}$ ng)			
	B1 (fresh air)	B2 ( <i>P. camemberti</i> )	B3 ( <i>P. caseifulvum</i> )	B4 (mix)
Q1	11 $\pm$ 1	12 $\pm$ 1	13 $\pm$ 2	13 $\pm$ 0
Q2	11 $\pm$ 1	12 $\pm$ 1	13 $\pm$ 1	13 $\pm$ 0

### System Outputs

Fig. 3 shows that Q1 has better adsorption-desorption reproducibilities than Q2. The frequency recovers to the initial baseline ( $f_0$ ). The frequency shifts  $\Delta f$  increase with the increasing bioaerosols concentration. According to Fig. 3, the highest  $\Delta f$  is referred to as Q1. The most  $\Delta f$  is detected on B2, B3, and B4 for Q1. The average peak  $\Delta f$  of Q1-B2, Q1-B3, and Q1-B4 are 423, 430, and 447 Hz, respectively. Q1-B1, which was exposed to the filtered fresh air, has a smaller  $\Delta f$  (337 Hz) than other Q1 groups exposed to bioaerosol samples. Similar treatments were also applied in Q2. Q2-B1 has only 187 Hz of  $\Delta f$ , which is smaller than Q1-B1. This result indicates that the coated QCM sensor has a better response than the uncoated one.

### System Performances

According to the equation below,  $\Delta f$  is influenced by the deposited bioaerosol sample mass ( $m$ , g) on the sensor's surface.  $A$  is the electrode surface area ( $0.196 \text{ cm}^2$ ), while  $\mu_Q$  and  $\rho_Q$  are the shear modulus ( $2.947 \times 10^{11} \text{ g/cm s}^2$ ) and the density of the sensor ( $2.684 \text{ g/cm}^3$ ), respectively.

$$\Delta m = [A \cdot \Delta f \cdot (\rho_q \cdot \mu_q)^{1/2}] / [2f_0^2] \quad (3)$$

The correlation between  $\Delta m$  and  $\Delta f$  is valid only if  $\Delta f \ll f_0$ . The calculated masses on Q1 for B1, B2, B3, and B4 are  $(12 \pm 1) \times 10^{-4}$ ;  $(15 \pm 1) \times 10^{-4}$ ;  $(15 \pm 0) \times 10^{-4}$ ; and  $(16 \pm 0) \times 10^{-4}$  ng, respectively. Q2-B1 and Q2-B2 generate  $(7 \pm 3) \times 10^{-4}$  and  $(9 \pm 0) \times 10^{-4}$  ng. No significant results are found at Q2 using B3 and B4, generating  $(9 \pm 1) \times 10^{-4}$ ; and  $(8 \pm 0) \times 10^{-4}$  ng of the deposited masses. There are more deposited masses on the surface of the coated QCM. Although the deposited masses are varied, there is no significant difference in the sensitivity between Q1 and Q2 ( $p = 0.43$ ). According to Eq. (1), the sensitivities are varied from  $23 \times 10^{-2}$  to  $29 \times 10^{-2} \text{ Hz/ng}$ .

Furthermore, this study also approaches the accuracy of the developed system by comparing the results with the calibrated measurement device. Compared to the Digital Dust Monitor, the developed system has 82% and 66% accuracy for the coated and uncoated sensors, respectively. These values interpret that the developed system has an accuracy of 82% to measure bioaerosol concentrations when using Q1, with the mean sensitivity of  $(28 \pm 1) \times 10^{-2} \text{ Hz/ng}$ . On the other hand, Q2 gives a lower accuracy, 66%, than Q1. Q2 also has a lower sensitivity ( $(27 \pm 3) \times 10^{-2} \text{ Hz/ng}$ ) than Q1.

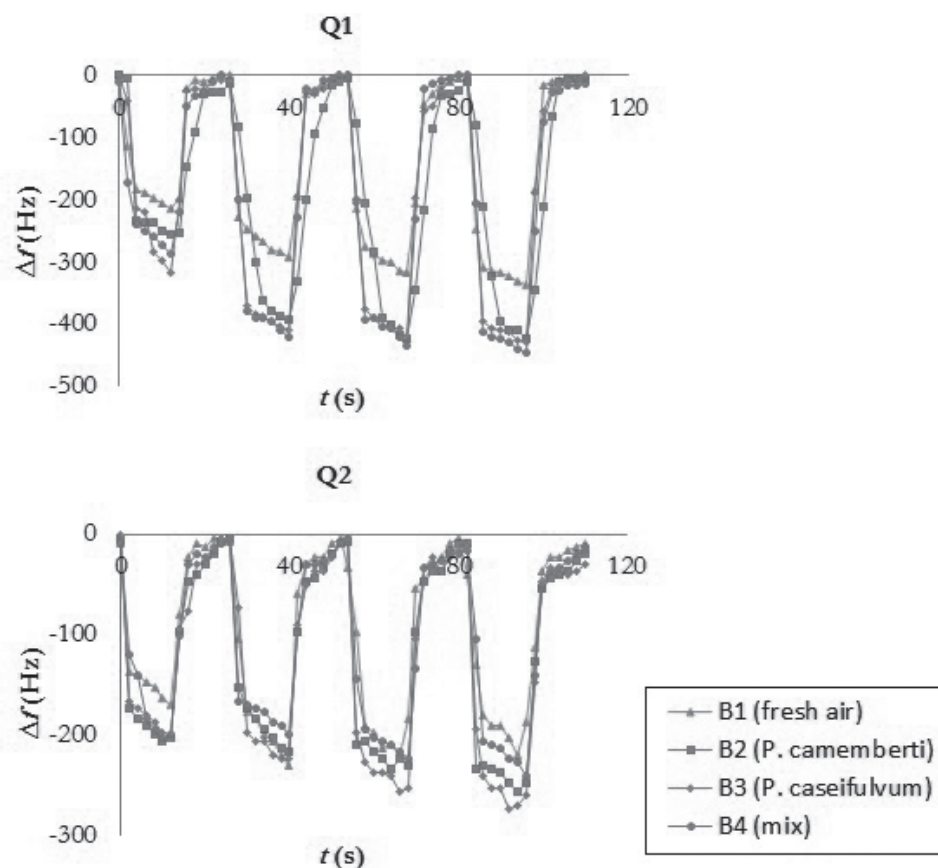


Fig. 3. Output response curves ( $\Delta f$ ) of: Q1 (GO-coated QCM) and Q2 (uncoated QCM).

## Discussion

A QCM can be used as a well-established biosensor, as developed by a previous study to detect vaccinia virus DNA [22]. In this section, the use of nanoparticles or another surface modification method in material sciences proved to be a good sensing ability technique, whether using electrochemical, magnetic, or piezoelectric sensors. The system's selectivity, sensitivity, feasibility, and response time are influenced by many factors, such as the coating material, layer, deposition technique, and many others [12, 25-27]. This study uses the system to measure the bioaerosol concentrations with various biosamples. The use of different QCMs is to identify the performance of the coated-QCM compared to the uncoated one. The results are obtained from the estimation of change in the resonance frequency of QCMs under different exposures to bioaerosol samples (B2-B4). The decrease in  $f$  (represented by  $\Delta f$ ) is considered proportional to the deposited substances (bioaerosols, represented by  $\Delta m$ ) on QCM's surface [12, 26, 27]. Thus, there will be a different result between coated and uncoated-QCMs.

As an alternative method in sensing particulate matters, whether bio or non-bio aerosols, the uses of GO as the coating material for the QCMs are investigated in this study. The specific GO coating

was chosen because its large surface area might cause more volatile or aromatic substances of the samples to be adsorbed on these active sites [15]. GO has rich hydrophilic functional groups (carboxyl, hydroxyl, and epoxy), which may increase the active and specific surface area [12]. For this reason, the swelling effect and the accumulation of the samples on the QCM's surface become important points. Fortunately, GO inherently represents a good mechanical modulus and a high hydrophilic surface area, which may cause a small probability of the swelling effect [16].

Moreover, GO has an antibacterial substance that may influence the GO-coated QCM. As well explained in a previous study, the interaction between chitosan chloride-GO composites and gram-negative bacteria *E. coli* and gram-positive bacteria *S. aureus* was investigated [29]. In this study, the used materials generated antibacterial properties that were inactive. GO can potentially be an anti-fungi and anti-bacteria when combined with phosphoramidate as a nanocomposite [30]. The interaction of this mechanism may exist in aromatic substances and epoxy groups of GO and cause plasma membrane damage and cell death [30]. GO may cause extreme damage to fungal cell walls and destroy cellular organelles [31]. As expected, these previous studies support the results of this study, resulting in a better performance of a GO-coated QCM than the uncoated one. As seen in the results, the highest frequency shift

is obtained at Q1. The value of  $\Delta f$  in Q1 is higher than the value in Q2 for all bioaerosol samples.

In addition to bioaerosols detection, GO has also been developed for other applications. As a composite, GO (with polydopamine) has been developed as a good humidity sensing device due to its ultra-sensitive behavior in water contents [12]. Another study also uses GO for the QCM coating materials and develops it as a humidity sensor [16]. As found in a previous study, GO/TiO<sub>2</sub> composites are deposited on the QCM's surface as a gas sensor [15]. In this study, GO alone gives a good sensitivity for gases and vapors detection compared to TiO<sub>2</sub>.

As reviewed before, QCMs are proven application-oriented sensors that can detect a wide range of bioaerosols [13]. Similarly, GO-coated QCM has a better performance than the uncoated QCM in sample detection. The GO-coated QCM has a better mass change, resulting in more  $\Delta f$  than the uncoated one. Our results are supported by many previous studies that the uncoated QCM cannot bind hydrophilic molecules or other substances due to its hydrophobicity [32]. For this reason, the silver surface must be modified with a hydrophilic structure to optimize the crystal. As expected, the GO-coated QCM has better accuracy (82%) than the uncoated one (66%) for fungal spore sensing.

Apart from these two parameters, data on the system performance and dissipation energy factor can become additional attractions of QCM. Our system results can be used as a preliminary study to develop a better GO treatment. There is a limitation like the coating material used in our developed system. The sensors need to be optimized under many further treatments. There are also limitations like sensitivity and selectivity limits with other substances, compatibility in differing each bioaerosol sample, and response time.

## Conclusions

This study develops a fungal spore mass measurement system based on graphene oxide coated QCM. The developed system shows a good performance with  $27 \times 10^{-2}$  to  $29 \times 10^{-2}$  Hz/ng sensitivity and  $23 \times 10^{-2}$  to  $29 \times 10^{-2}$  Hz/ng for coated and uncoated sensors, respectively. The best performance is obtained from the GO-coated QCM sensor. The system works well in measuring fungal spore mass with an accuracy of 82% (GO coated QCM) and 66% (uncoated QCM). The coated QCM has the prospects of being developed as a fungal spore sensor.

## Acknowledgments

All authors offer special thanks to the Institute of Research and Community Services Brawijaya University (LPPM) and the Ministry of Research and

Technology/ National Research and Innovation Agency Republic of Indonesia for their financial contribution (Contract number: 023/E4.1/AK.04.PT/2021).

## Conflict of Interest

The authors declare no conflict of interest.

## References

- MORGADO-GAMERO W.B., PARODY A., MEDINA J., RODRIGUEZ-VILLAMIZAR L.A., AGUDELO-CASTAÑEDA D. Multi-antibiotic resistant bacteria in landfill bioaerosols: Environmental conditions and biological risk assessment. *Environmental Pollution* **290**, 118037, **2021**.
- XU J., JIA C., HE J., XU H., TANG Y., JI D., YU H., XIAO H., WANG C. Biomass Burning and fungal spores as sources of fine aerosols in Yangtze River Delta, China – using multiple organic tracers to understand variability, correlations and origins. *Environmental Pollution* **251**, 155, **2019**.
- BARNES C.S., DOWLING P., OSDOL T.V., PORTNOY J. Comparison of indoor fungal spore levels before and after professional home remediation. *Annals of Allergy, Asthma and Immunology* **98** (3), 262, **2007**.
- MOUSAVI B., HEDAYATI M.T., HEDAYATI N., ILKIT M., SYEDMOUSAVI S. Aspergillus species in indoor environments and their possible occupational and public health hazards. *Current Medical Mycology* **2** (1), 36, **2016**.
- THAM R., ERBAS B., DHARMAGE S.C., TANG M.L.K., ALDAKHEEL F., LODGE C.J., THOMAS P.S., TAYLOR P.E., ABRAMSON M.J., LOWE A.J. Outdoor fungal spores and acute respiratory effects in vulnerable individuals. *Environmental Research* **178**, 108675, **2019**.
- BAXI S.N., SHEEHAN W.J., SORDILLO J.E., MUILENBERG M.L., ROGERS C.A., GAFFIN J.M., PERMAUL P., LAI P.S., LOUISIAS M., PETTY C.R., FU C., GOLD D.R., PHIPATANAKUL W. Association between fungal spore exposure in inner-city schools and asthma morbidity. *Annals of Allergy, Asthma and Immunology* **122** (6), 610, **2019**.
- OLANIYAN T., DALVIE M.A., RÖÖSLI M., NAIDOO R.N., KÜNZLI N., HOOGH K.D., BERMAN D., PARKER B., LEANER J., JEEBHAY M.F. Short term seasonal effects of airborne fungal spores on lung function in a panel study of schoolchildren residing in informal settlements of the Western Cape of South Africa. *Environmental Pollution* **260**, 114023, **2020**.
- GÉRY A., DELANOË A., HEUTTE N., CHOSSON E., BONHOMME J., GARON D. A novel qPCR based-method for detection and quantification of three recurrent species of *Penicillium* isolated from bioaerosols in mold-damaged homes. *Journal of Microbiological Methods* **186**, 106236, **2021**.
- FERGUSON R.M.W., NEATH C.E.E., NASIR Z.A., GARCIA-ALCEGA S., TYRREL S., COULON F., DUMBRELL A.J., COLBECK I., WHITBY C. Size fractionation of bioaerosol emissions from green-waste composting. *Environment International* **147**, 106327, **2021**.
- LIAO L., BYEON J.J., PARK J.H. Development of a size-selective sampler combined with an adenosine triphosphate

- bioluminescence assay for the rapid measurement of bioaerosols. *Environmental Research* **194**, 110615, **2021**.
11. BROUSSEAU L.M., DONALD V., RICE N., GOODELL K., NELLIS M., HAIRSTON P. Differences in detected fluorescence among several bacterial species measured with a direct-reading particle sizer and fluorescence detector. *Aerosol Science and Technology* **32** (6), 545, **2020**.
  12. ZHANG D., SONG X., WANG Z., CHEN H. Ultra-highly sensitive humidity sensing by polydopamine/graphene oxide nanostructure on quartz crystal microbalance. *Applied Surface Science* **538**, 147816, **2021**.
  13. JANDAZ P.J., PRABAKARAN K., LUO J., HOLADAY D. Effective utilization of quartz crystal microbalance as a tool for biosensing applications. *Sensors and Actuators A: Physical* **331**, 113020, **2021**.
  14. GIANNELI M., YAN Y., POLO E., PEIRIS D., AASTRUP T., DAWSON K.A. Novel QCM-based method to predict in vivo behaviour of nanoparticles. *Procedia Technology* **27**, 197, **2017**.
  15. JAYAWARDENA S., KUBONO A., RAJAPAKSE R.M.G., SHIMOMURA M. Effect of titanium precursors used in the preparation of graphene oxide/TiO<sub>2</sub> composite for gas sensing utilizing quartz crystal microbalance. *Nano-Structures & Nano-Objects* **28**, 100780, **2021**.
  16. HO C.Y., WU Y.S. Diamine decorated graphene oxide film on quartz crystal microbalance for humidity-sensing analysis. *Applied Surface Science* **510**, 145257, **2020**.
  17. YANG M., HE J. Graphene oxide as quartz crystal microbalance sensing layers for detection of formaldehyde. *Sensors and Actuators, B: Chemical* **228**, 486, **2016**.
  18. BUDIANTO A., WARDOYO A.Y.P., MASRUROH M., DHARMAWAN H.A., NURHUDA M. Performance test of an aerosol concentration measurement system based on quartz crystal microbalance. *Journal of Physics: Conference Series* **1811**, 012033, **2021**.
  19. JANKOWSKA E.J., REPONEN T., WILLEKE K., GRINSHUPUN S.A., CHOI K.J. Collection of fungal spores on air filters and spore reentrainment from filters into air. *Journal of Aerosol Science* **31** (8), 969, **2000**.
  20. MADHWAL S., PRABHU V., SUNDRIYAL S., SHRIDHAR V. Ambient bioaerosol distribution and associated health risks at a high traffic density junction at Dehradun City, India. *Environmental Monitoring and Assessment* **192** (3), 156, **2020**.
  21. LEE J.H., HWANG G.B., JUNG J.H., LEE D.H., LEE B.U. Generation characteristics of fungal spore and fragment bioaerosols by airflow control over fungal cultures. *Journal of Aerosol Science* **41** (3), 319, **2010**.
  22. KLEO K., KAPP A., ASCHER L., LISDAT F. Detection of vaccinia virus DNA by quartz crystal microbalance. *Analytical Biochemistry* **418** (2), 260, **2011**.
  23. WARDOYO A.Y.P., JUSWONO U., NOOR J.A.E. The association between the diesel exhaust particle exposure from bus emission and the tubular epithelial cell deformation of rats. *Environmental Science and Pollution Research* **27**, 23073, **2020**.
  24. JIN H., TAO X., FENG B., YU L., WANG D., DONG S., LUO J. A humidity sensor based on quartz crystal microbalance using graphene oxide as a sensitive layer. *Vacuum* **140**, 101, **2017**.
  25. MADHWAL S., PRABHU V., SUNDRIYAL S., SHRIDHAR V. Distribution, characterization and health risk assessment of size fractionated bioaerosols at an open landfill site in Dehradun, India. *Atmospheric Pollution Research* **11** (1), 156, **2020**.
  26. TRIYANA K., SEMBIRING A., RIANJANU A., HIDAYAT S.N., RIOWIRAWAN R., JULIAN T., KUSUMAATMAJA A., SANTOSO I., RORO R. Chitosan-based quartz crystal microbalance for alcohol sensing. *Electronics (Switzerland)* **7** (9), 1, **2018**.
  27. SAKTI P.S., MASRUROH, KAMASI D.D., KHUSNAH N.F. Stearic acid coating material loading effect to quartz crystal microbalance sensor. *Materials Today: Proceedings* **13**, 53, **2019**.
  28. JAYAWARDENA S., SIRIWARDENA H.D., RAJAPAKSE R.M.G., KUBONO A., SHIMOMURA M. Fabrication of a quartz crystal microbalance sensor based on graphene oxide/TiO<sub>2</sub> composite for the detection of chemical vapors at room temperature. *Applied Surface Science* **493**, 250, **2019**.
  29. LI X., SUN J., CHE Y., LV Y., LIU F. Antibacterial properties of chitosan chloride-graphene oxide composites modified quartz sand filter media in water treatment. *International Journal of Biological Macromolecules* **121**, 760, **2019**.
  30. GHOLIVAND K., MARYAM R.D., ARDEBILI A., ALIREZA S., MOHAMMADPOUR M., ALI ASHGAR E.V. New graphene oxide-phosphoramidate nanocomposites as practical tools for biological applications including anti-bacteria, anti-fungi and anti-protein. *Journal of Molecular Structure* **1240**, 130528, **2021**.
  31. HOOK A.L., CHANG C.Y., YANG J., LUCKETT J., COCKAYNE A., ATKINSON S., MEI Y., BAYSTON R., IRVINE D.J., LANGER R., ANDERSON D.G., WILLIAMS P., DAVIES M.C., ALEXANDER M. Combinatorial discovery of polymers resistant to bacterial attachment. *Nature Biotechnology* **30** (9), 868, **2012**.
  32. YILMAZ M., BAKHSHPOUR M., GÖKTÜRK I., PIŞKIN A.K., DENIZLI A. Quartz crystal microbalance (QCM) based biosensor functionalized by HER2/Neu antibody for breast cancer cell detection. *Chemosensors* **9** (4), 80, **2021**.